Installation Instructions

9A31500* Welch Allyn Light Bracket

(Use w/ 48700 Light)

Intended Use

To mount a Welch Allyn 48700 Light to 222 exam table *(on patient's left side)*.

Kit Components

Description	*Part Number*	*Qty*
Bracket	030-1429-50	1
Bottom Plate	050-5579-50	1
Screws:		
#10-24 x 1/2"	040-0010-129	4
#10-32 x 3/8"	040-0010-74	2
Nuts:		
#10-32, Esna thin	041-0010-12	2

Installation

(1) Insert bottom plate (1, Figure 1) thru slot in bracket (2) and secure with two 1/2" screws (3).

(2) Lift seat section; pull footrest and stirrups out.

(3) Remove screw (4) and insert front of bracket (2) between upperwrap & drawer housing.

(4) Align hole in bracket (2) with holes in upperwrap and drawer housing; then install screw (4).

(5) Remove screw (5) and move back of bracket (2) between upperwrap & drawer housing.

(6) Align hole in bracket (2) with holes in upperwrap and drawer housing; then install screw (5).

(7) Remove drawer.

(8) Secure bracket (2) to bottom of drawer housing with two 3/8" screws (6) and two nuts (7).

NOTE

There are two screws *(#10-24 x 1/2")* provided to mount the Welch Allyn 48700 light to the bracket.

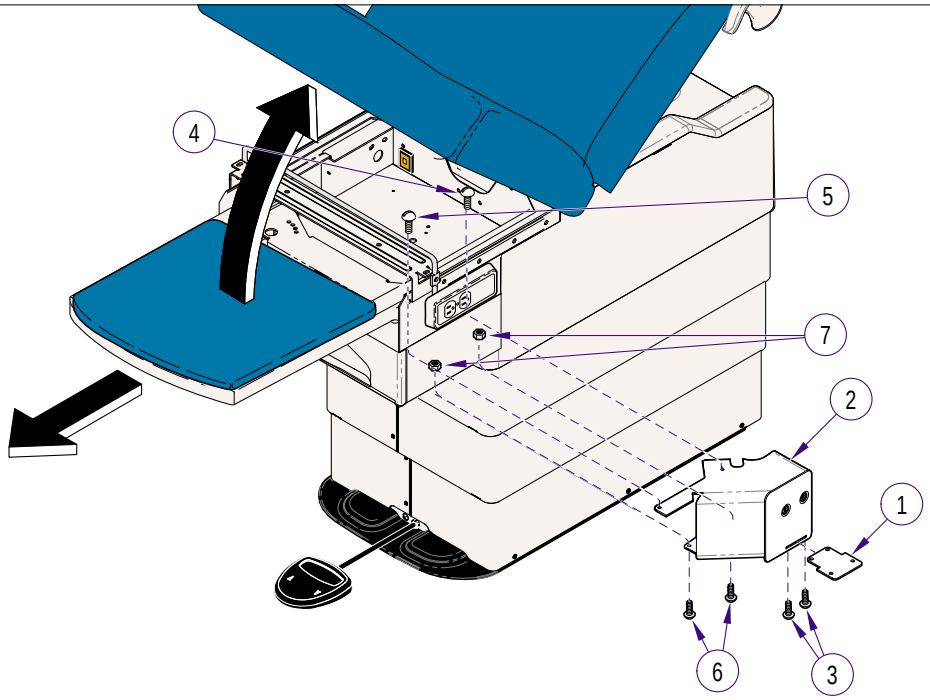

Figure 1. Welch-Allyn Bracket Installation

MA606500i

© Midmark Corporation 2002